



CERTIFICATE OF INSPECTION





Based upon the data below, Dual Mfg, Inc. **VERIFIES** that this sieve meets the requirements set forth by **ASTM E11-17** for nominal dimensions and permissible variations for sieve cloth and compliance, inspection and calibration test sieves.

The data for this Sieve was derived using a Nikon V-12B optical imaging device following internal work instructions. The Nikon V-12B, serial #1100935 was last calibrated on **06/01/2020** with calibration certificate of **06/01/2021**. Optical calibration was performed using standards 37876 #622, Cert#1117703; S2014-0001, Cert# 1117704; 895, Cert# 1117702. Above traceable to N.I.S.T. Test# CQG-4990-388188-00. Calibration Systems utilized complies with ISO/IEC17025-2005 Standard.

New Certification
 Re-Certification
 Sieve Usually Inspected
 Sieve Cleaned

Wire Diameter

Opening Size

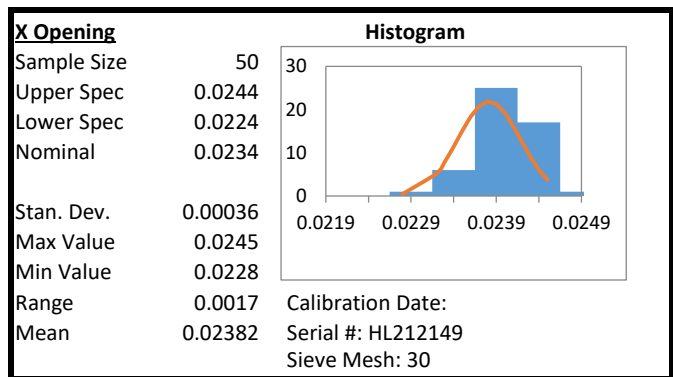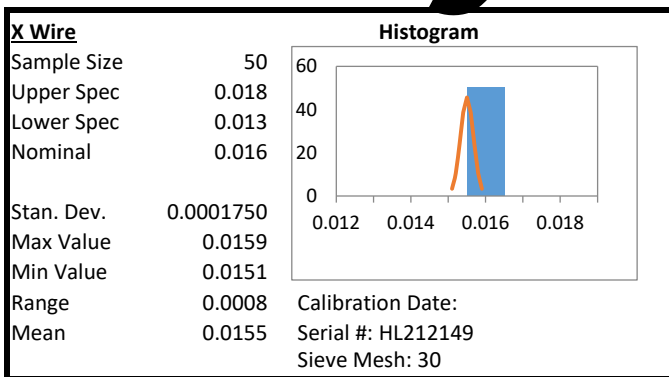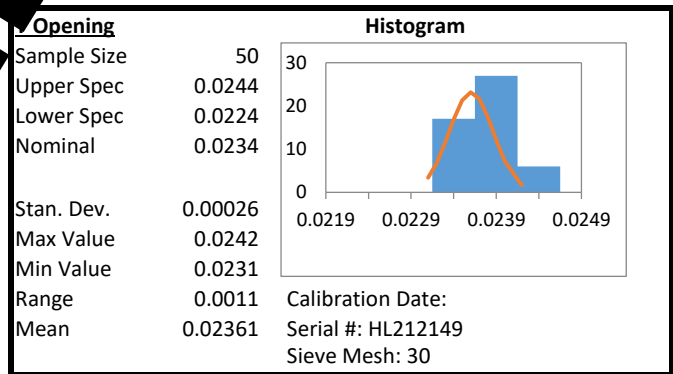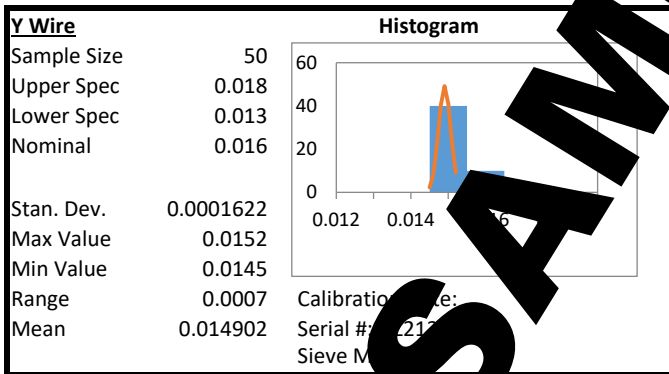

Laboratory Technician

4/6/2021

Date